

## Reference Material Certificate

# 124/04

Aluminium Base (Type of Standard)  
Al pure (99.95-99.8% Al), Set 120

### Certified Values

Element	Mass content [%]	Uncertainty [%]
Silicon (Si)	0.105	± 0.005
Iron (Fe)	0.145	± 0.005
Copper (Cu)	0.0533	± 0.0017
Manganese (Mn)	0.0540	± 0.0018
Magnesium (Mg)	0.0558	± 0.0017
Chromium (Cr)	0.0509	± 0.0018
Nickel (Ni)	0.0592	± 0.0018
Zinc (Zn)	0.0515	± 0.0015
Titanium (Ti)	0.0505	± 0.0019
Silver (Ag)	0.0190	± 0.0005
Boron (B)	0.0002	± 0.0001
Beryllium (Be)	0.0019	± 0.0001
Bismuth (Bi)	0.0151	± 0.0005
Calcium (Ca)	0.0003	± 0.0001
Cadmium (Cd)	0.0210	± 0.0006
Cerium (Ce)	0.0451	± 0.0018
Cobalt (Co)	0.0201	± 0.0008
Gallium (Ga)	0.0365	± 0.0016
Lanthanum (La)	0.0307	± 0.0009
Lithium (Li)	0.00060-0.00080	± 0.00005
Sodium (Na)	0.0014-0.0020	± 0.0002
Lead (Pb)	0.0232	± 0.0015
Antimony (Sb)	0.0252	± 0.0010
Tin (Sn)	0.0208	± 0.0012
Vanadium (V)	0.0449	± 0.0025
Zirconium (Zr)	0.0054	± 0.0004

The uncertainty reported is the result of standard deviation of all results multiplied with a factor of two and represents approximately the 95% confidence interval.

This certified reference material has elements with a range. Individually certified values for those elements are available on S-certificates only.

## Manufacturing

### Homogeneity

Homogeneity testing is performed by means of spark emission spectroscopy. Tests involve making multiple measurements on individual samples taken at regular intervals along the entire length of each cast rod. Depending on the mass content of the element, the relative standard deviation of multiple measurements between discs or within one disc is typically found between 0.3% - 1% for alloying and other elements and 0.5% - 5% for trace elements.

### Analysis

The values listed in this analysis certificate are the results of multiple analyses performed in our chemical analysis laboratory which is an accredited test facility for aluminium alloys according to the international standard ISO 17025. The analyses are based on established wet chemical procedures.

### Description of Sample


This reference material is available in the form of discs (approx. Ø 60 x 25 mm).

### Intended use and Stability

This certified reference material is primarily intended for use in spark optical emission spectroscopy. Other applications are X-ray fluorescence spectrometry (XRF) and classical wet chemical procedures. The minimum sample size for wet chemical analysis is 0.2g. The material will remain stable for the period given below (certification validity) if it is stored in a dry and clean environment at room temperature.

### Instructions for Use

Calibration measurements should be made within a ring between 2mm and 22mm from the edge of the CRM face. For wet chemical analysis chips have to be prepared by turning or milling of the sample surface.

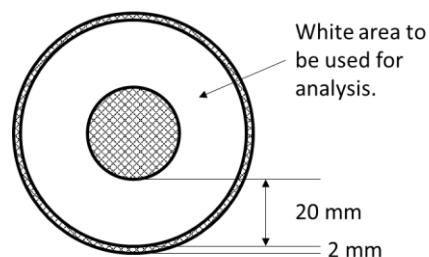

### Traceability

Traceability of the certified mass contents to the SI (Système International d'Unités) is ensured by calibration using certified standard solutions or pure metals or substances of known stoichiometry.



Dr. Benedikt Moser  
CTO



Patrik Bachmann  
Head of Inorganic Analytics

Suisse Technology Partners Ltd.  
Querstrasse 5  
8212 Neuhausen am Rheinfall  
Switzerland

Phone: +41 52 551 11 00  
Fax : +41 52 551 11 99  
Email: [refmat@suisse-tp.ch](mailto:refmat@suisse-tp.ch)  
Internet: <https://reference-materials.ch>

Date of certification: 13-Feb-2003  
Certificate version 003: 04-Jan-2022  
This certificate is valid until: Feb-2078